


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: LAURIC D23 ACID

HPLC

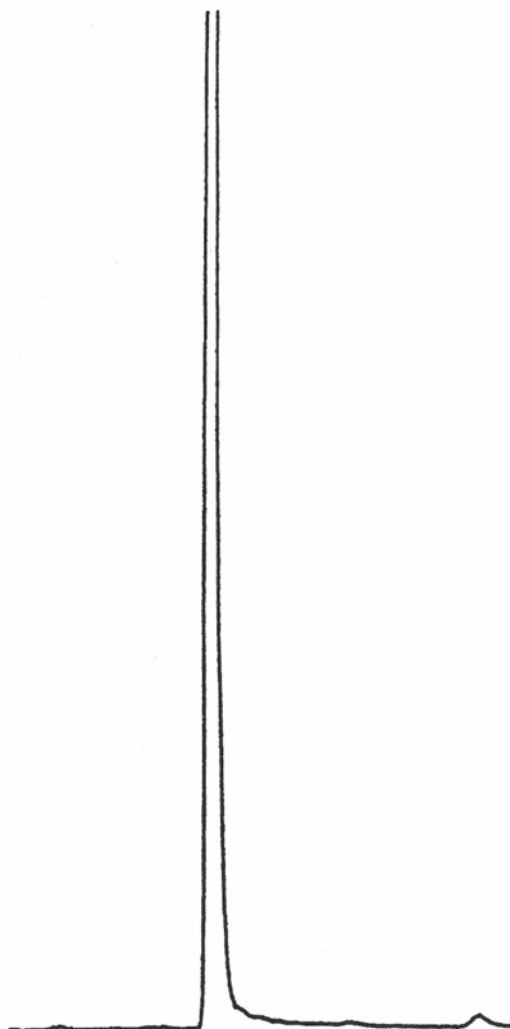

CONDITIONS

| | |
|-----------------|---|
| Column | <i>Zorbax ODS 250 x 4.6 mm</i> |
| Injected Volume | <i>20 µl</i> |
| Eluent | <i>Acetone 45% /(Methanol 50 + water 49.5/0.5% Acetic Acid)55 %</i> |
| Flow Rate | <i>1.5 ml/min</i> |
| Pressure | <i>2.5 bars</i> |
| Gas | <i>Helium</i> |
| Temperature | <i>Detector 50° C, Column 35° C</i> |

S.E.D.E.R.E.

PARC VOLTA - BP 27

9, rue Parmentier

94141 Alfortville Cedex FRANCE

Application #40