


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: POLYETHYLENE GLYCOL 1450

HPLC
Gradient

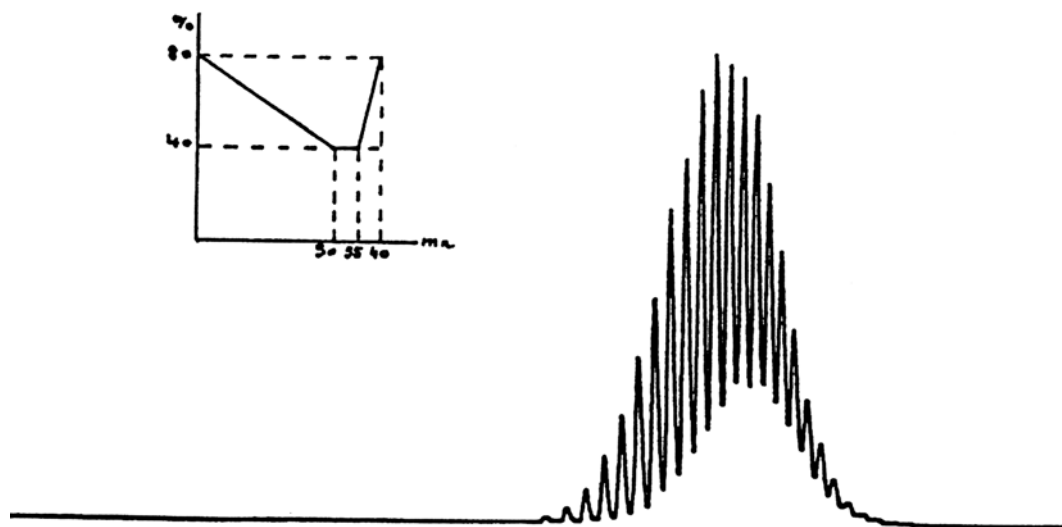

**Gradient: 80% to 40% in 30 min
Hold at 40 % for 5 min
40 % to 80 % in 5 min**

CONDITIONS

Column	<i>Nucleosil 120-7-C18 250 x 4 mm.</i>
Eluent	<i>A: Water/Methanol (95/5) [w/w] B: Methanol/Water (95/5) [w/w]</i>
Flow Rate	<i>1.0 ml/min</i>
Temperature	<i>36° C</i>