


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: ORGANIC ACIDS

HPLC

1 = Malic Acid
2 = Succinic Acid
3 = Fumaric Acid
4 = Aconitic Acid

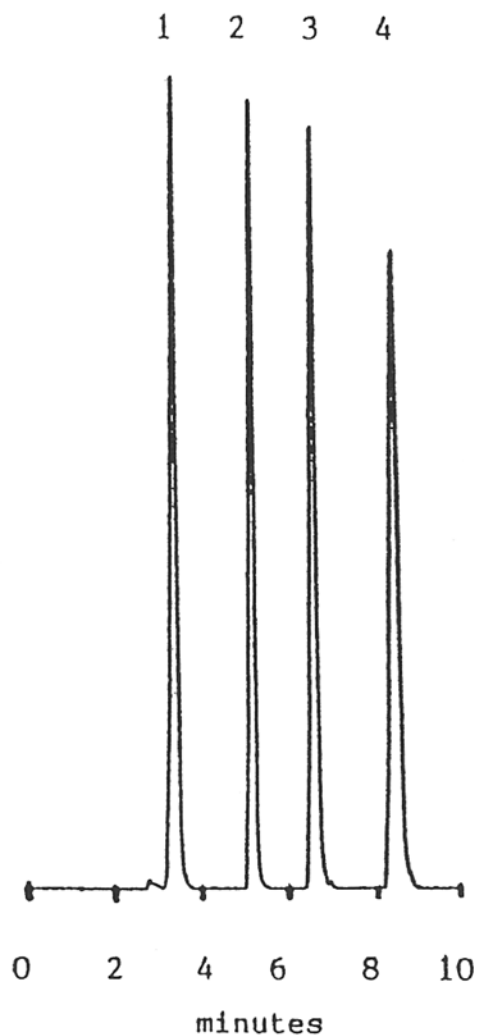

CONDITIONS

Column	<i>Inertsil ODS, 5 μ (250 x 4.6 mm)</i>
Injected sample	<i>20 μl (approximately 1 μg/μl each)</i>
Eluent	<i>0.1% TFA (aqueous) MeOH (90/10)</i>
Flow Rate	<i>1 ml/min</i>
Pressure	<i>2.2 bars</i>
Gas	<i>Nitrogen</i>
Temperature	<i>50° C</i>

Analyzed By : Richard Scientific, Novato CA 94949 USA