


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: SOY FATTY ACID DISTILLATE

HPLC
Gradient

- 1 = Linolenic Acid (18:3)
- 2 = Linoleic Acid (18:2)
- 3 = Oleic Acid (18:1)
- Palmitic Acid (16:0)
- 4 = Stearic Acid (18:0)
- 5 = δ -Tocopherol
- 6 = γ, β -Tocopherols
- 7 = α -Tocopherol
- 8 = Stigmasterol

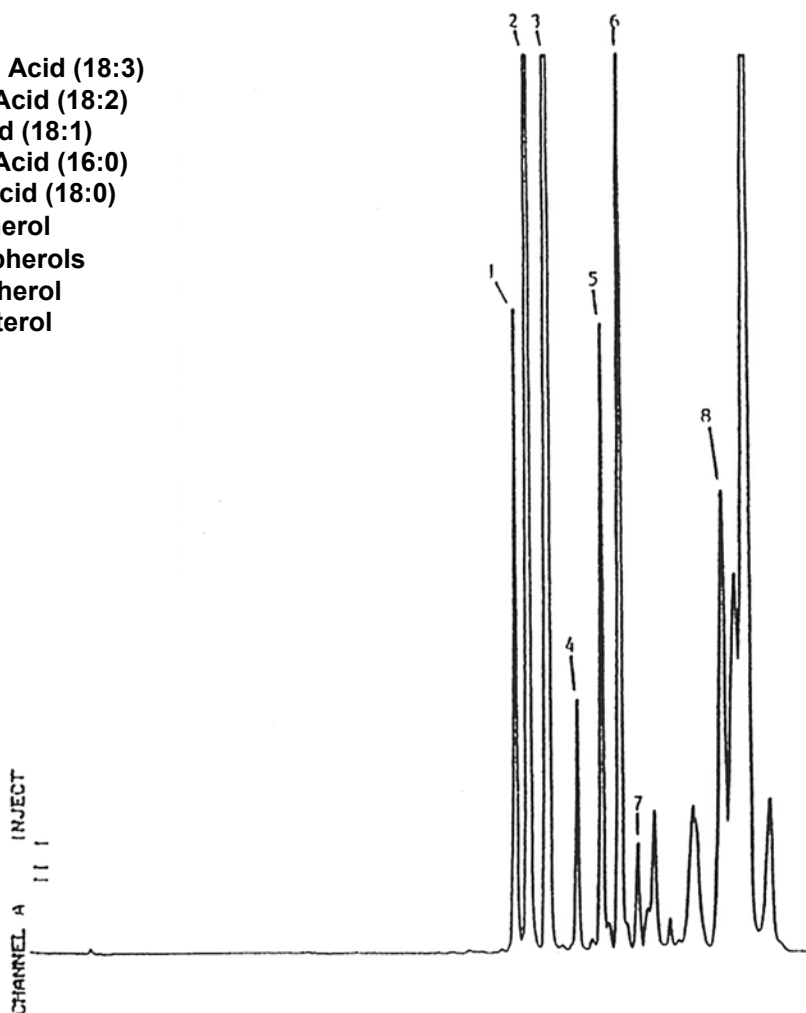

Gradient : 20% B to 100% B in 15 min.
Hold 15 min.

CONDITIONS

Column	<i>Kromasil ODS, 5 μ</i> <i>(250 x 4.6 mm)</i>
Injected sample	<i>200 μg</i>
Eluent	<i>A : 0.1% Aqueous TFA/MeOH (90/10)</i> <i>B : Methanol/Acetone (60/40)</i>
Flow Rate	<i>1.0 ml/min</i>
Pressure	<i>2.2 bars</i>
Gas	<i>Nitrogen</i>
Temperature	<i>45° C</i>

Analyzed By : Richard Scientific, Novato CA 94949 USA

S.E.D.E.R.E.
PARC VOLTA - BP 27
9, rue Parmentier
94141 Alfortville Cedex FRANCE

Application #97