


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: α - and β -ESTRADIOL

HPLC

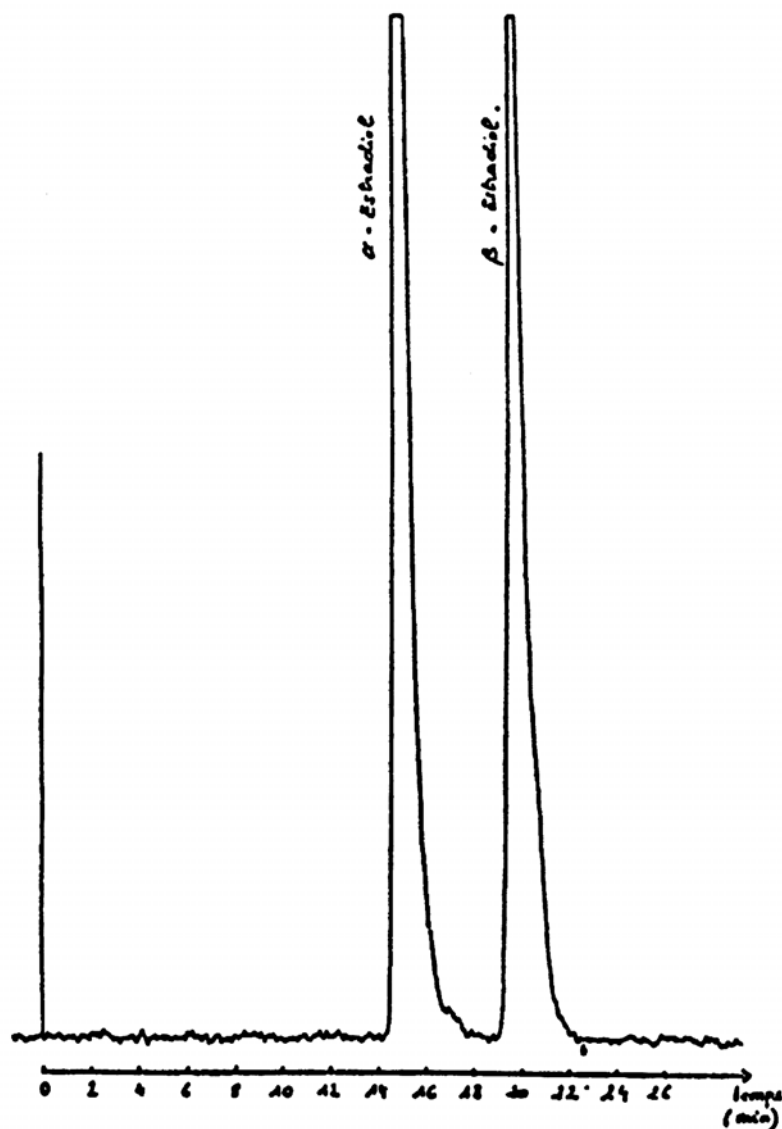

CONDITIONS

Column	Zorbax Sil - 5 μ m 25 x 4.6 mm
Injected Volume	20 μ l
Eluent	Cyclohexane/Ethyl Acetate (95/5)
Gas	Nitrogen
Temperature	35° C