


# SEDEX Low Temperature Evaporative Light Scattering Detector

## SAMPLE: TEST COLUMNS

HPLC  
Gradient

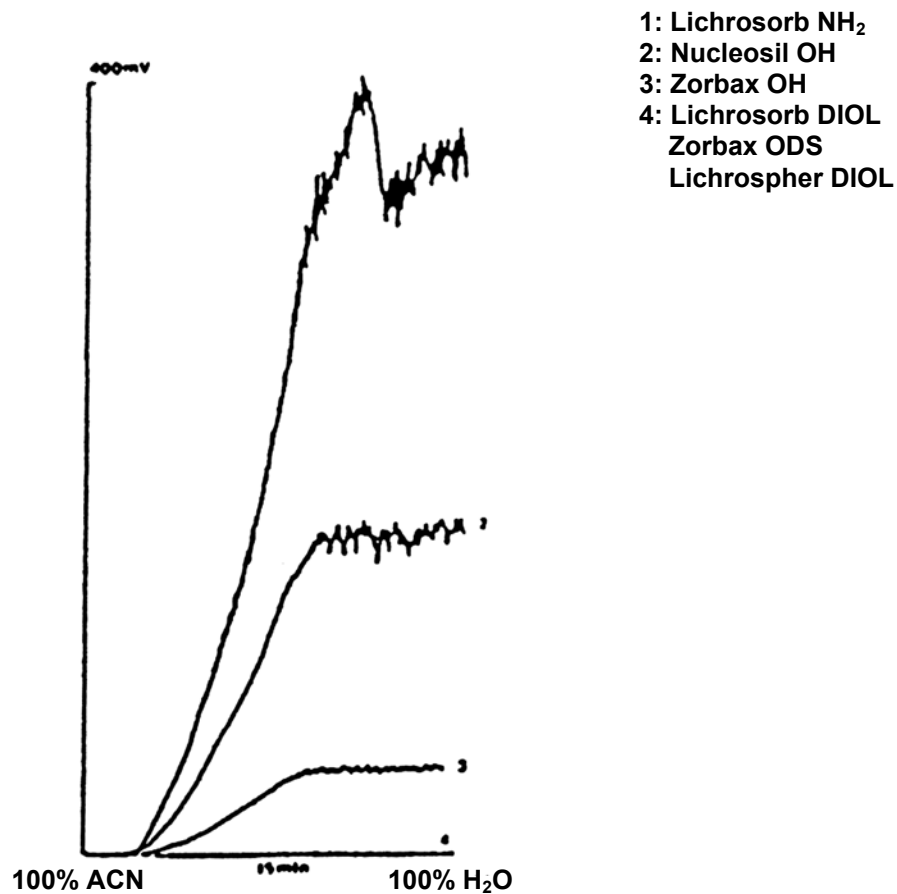

Gradient: 0-100 % Water in 15 min

### CONDITIONS

|             |                           |
|-------------|---------------------------|
| Column      | See above                 |
| Eluent      | A: Acetonitrile, B: Water |
| Flow Rate   | 2.0 ml/min                |
| Temperature | 45° C                     |