


**ION PAIR CHROMATOGRAPHY
OF INORGANIC ANIONS
SAMPLE : Standards**

HPLC

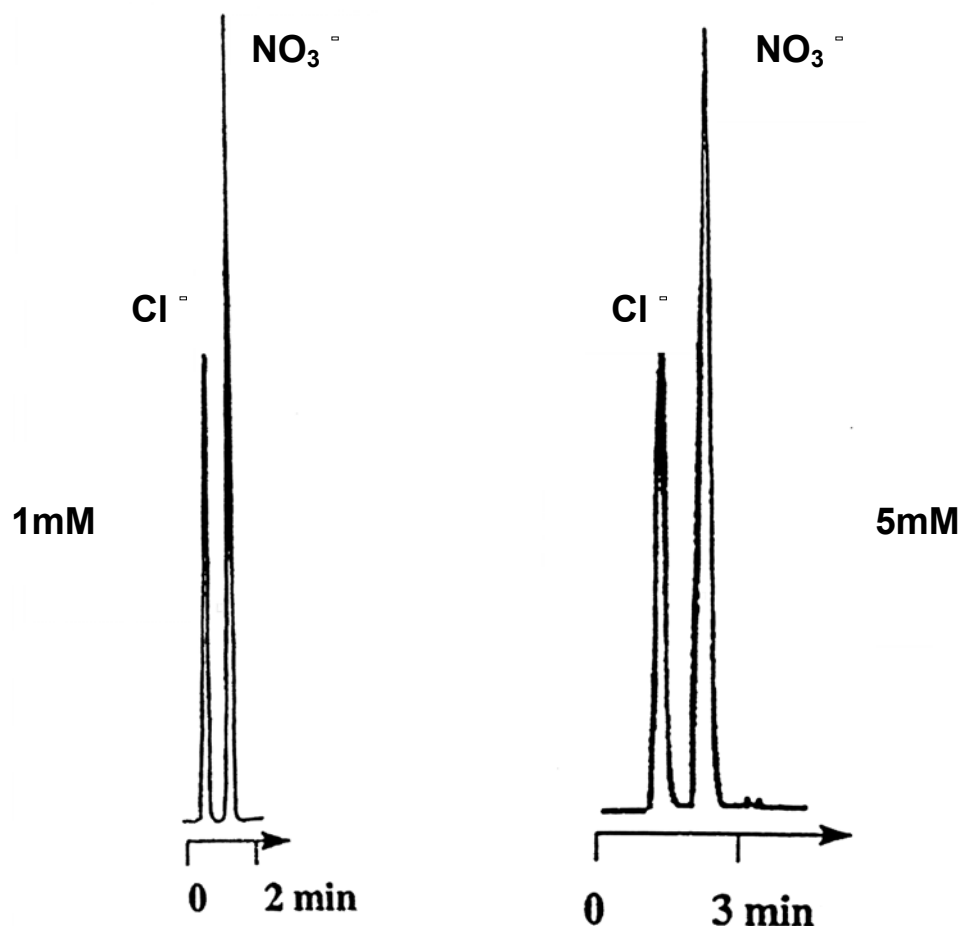

stationnary phase : C18
Mobile phase : Water with ion pairing agent (1 and 5 mM)
flow rate : 400 µl/min

CONDITIONS

Column	20 µl
Pressure	2 bars
Gas	Air
Gain	9
Temperature	40°C

Analyzed by : LCBA 45100 Orléans FRANCE